







ACOUSTICAL SYSTEMS - LLC

# FlutterFree® T Supplemental Random Incidence Absorption Data

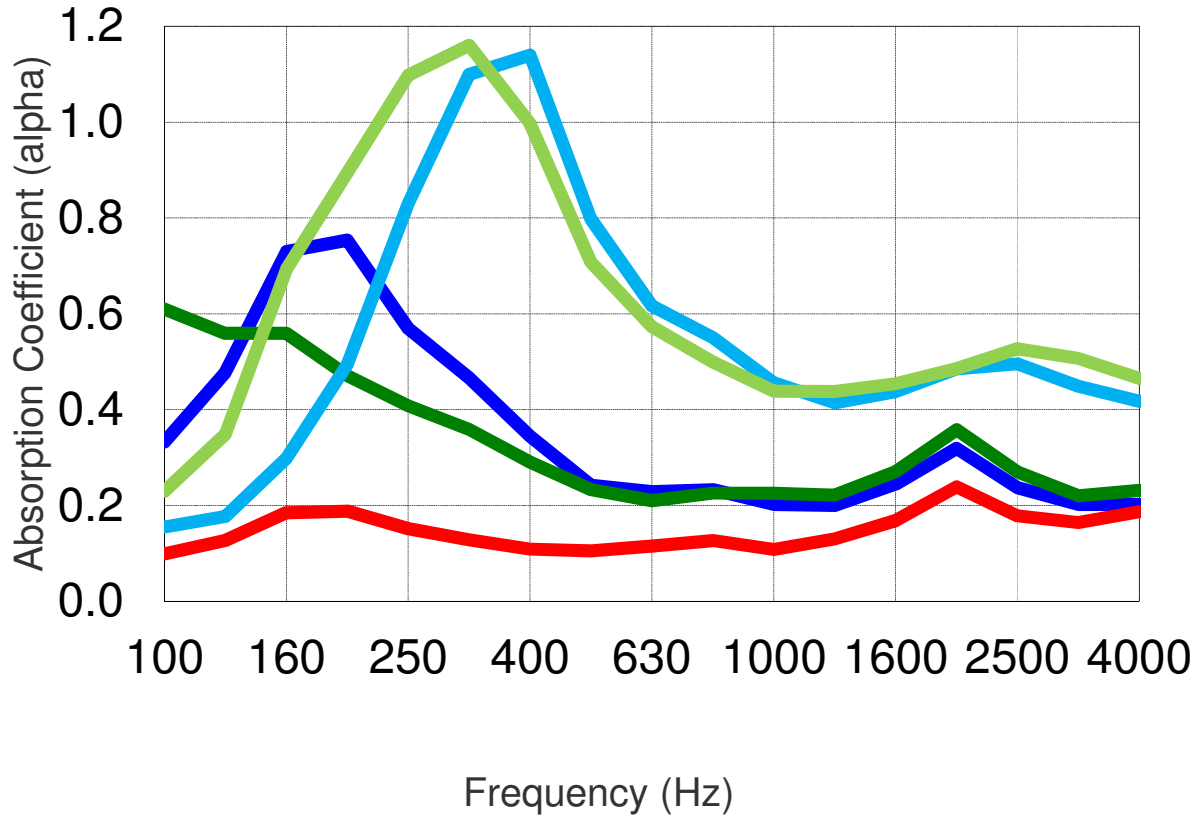

- C Mount w/ Helmholtz
- C Mount w/ Slots
- A Mount
- D Mount w/ Helmholtz
- D Mount w/ Slots

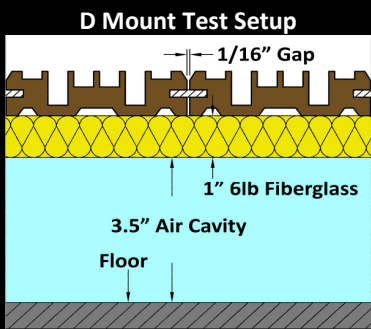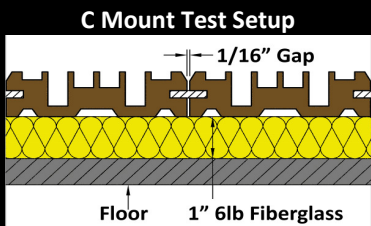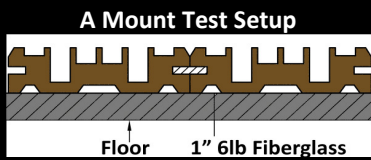

FREQ	A Mount	C Mount w/ Helmholtz	C Mount w/ Slots	D Mount w/ Helmholtz	D Mount w/ Slots
100	0.07	0.18	0.00	0.48	0.27
125	0.10	0.33	0.15	0.61	0.23
160	0.13	0.48	0.18	0.56	0.35
200	0.19	0.73	0.30	0.56	0.69
250	0.19	0.75	0.49	0.47	0.89
315	0.15	0.57	0.83	0.41	1.10
400	0.13	0.47	1.10	0.36	1.16
500	0.11	0.34	1.14	0.29	1.00
630	0.11	0.24	0.80	0.23	0.71
800	0.12	0.23	0.62	0.21	0.57
1000	0.13	0.23	0.55	0.23	0.50
1250	0.11	0.20	0.46	0.23	0.44
1600	0.13	0.20	0.41	0.22	0.44
2000	0.17	0.24	0.44	0.27	0.45
2500	0.24	0.32	0.49	0.36	0.49
3150	0.18	0.24	0.50	0.27	0.53
4000	0.16	0.20	0.45	0.22	0.51
5000	0.19	0.20	0.42	0.23	0.47